


OIM5002 SN3486 Bode X

Thursday, February 02, 2017

4:08 PM

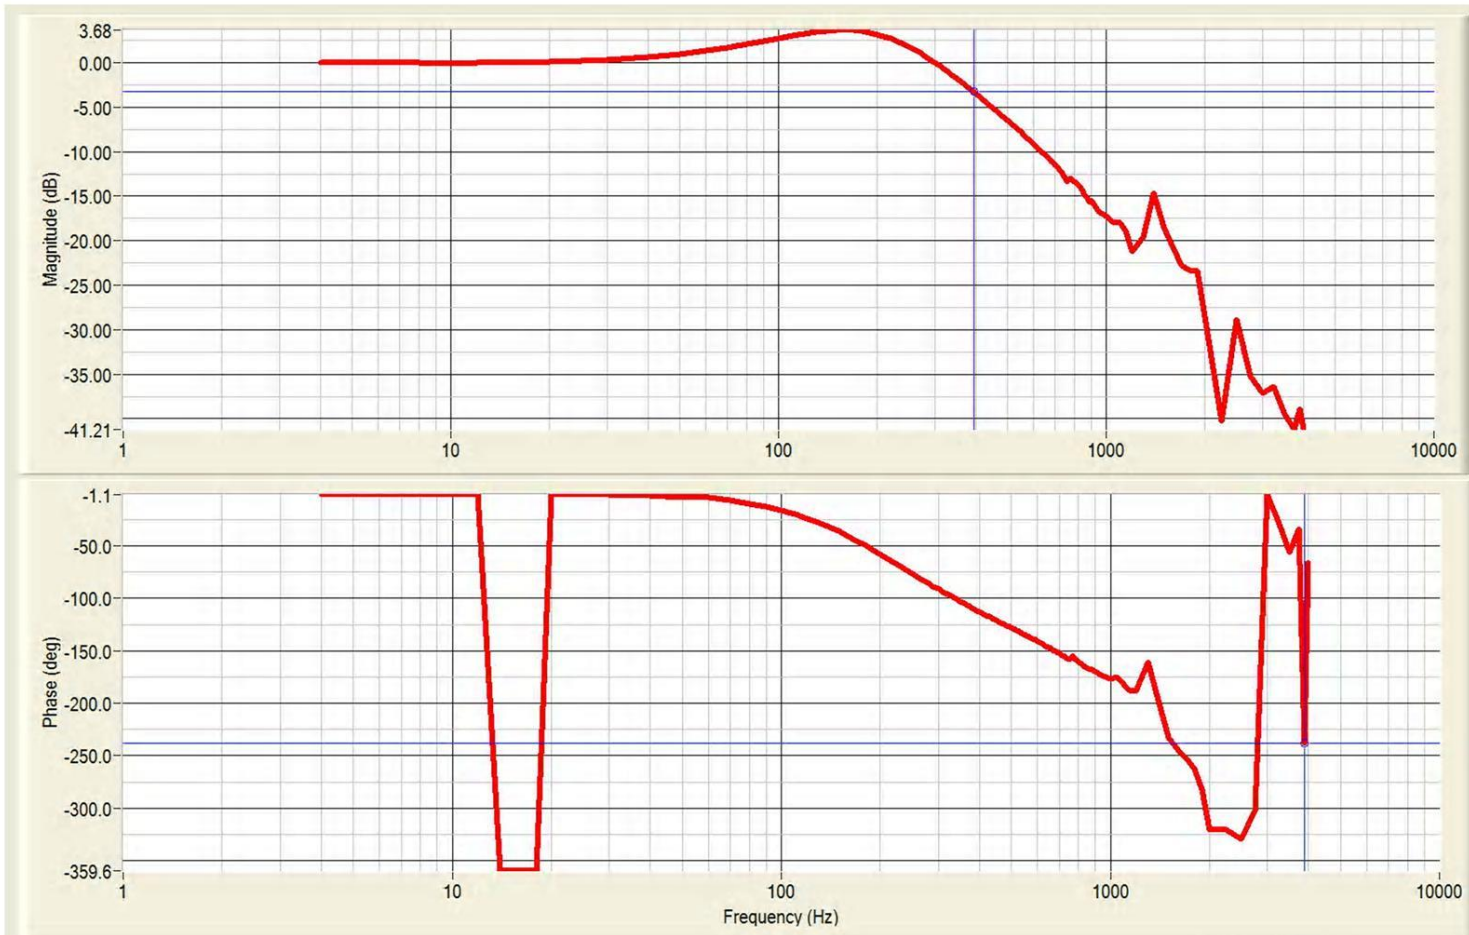

Closed Loop Error Rejection Open Loop

Frequency	Magnitude	Phase
4000.000	-41.153	-66.326

SN

X Axis Y Axis

START

PRINT

Cursor Position


Frequency (Hz)	Magnitude (dB)
395.000	-3.279

Frequency (Hz)	Phase (deg)
0.000	0.000

OIM5002 SN3486 Bode Y

Thursday, February 02, 2017

4:16 PM

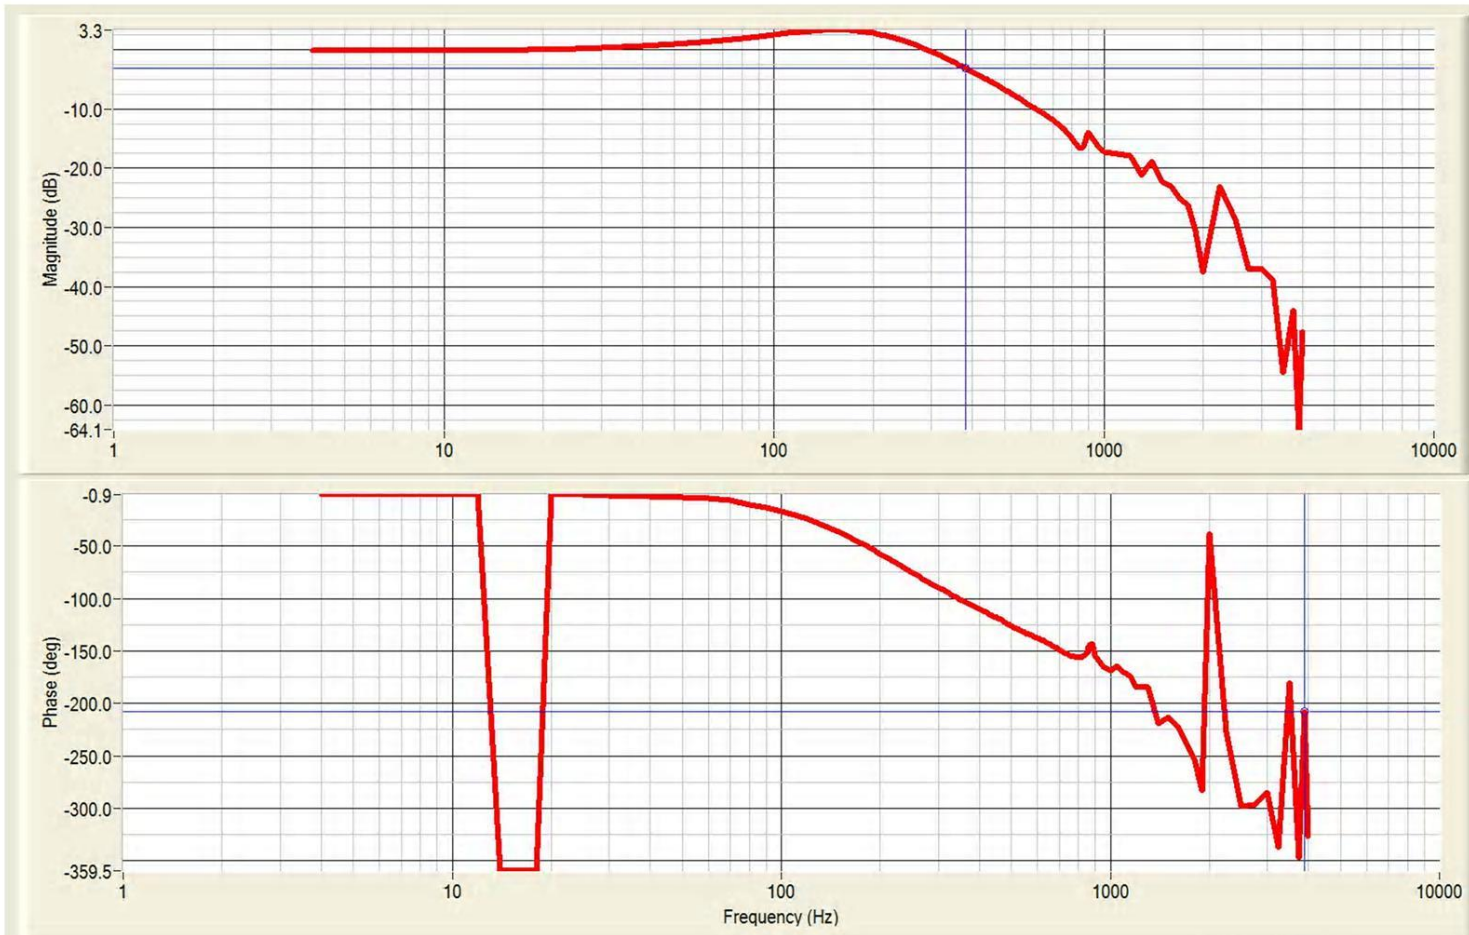

Cursor Position

Frequency (Hz)	Magnitude (dB)
380.000	-3.046
Frequency (Hz)	Phase (deg)
0.000	0.000

Closed Loop Error Rejection Open Loop

SN


Frequency	Magnitude	Phase
4000.000	-47.647	-326.586

X Axis Y Axis

OIM5002 SN3486 Small Step X

Thursday, February 02, 2017


4:21 PM

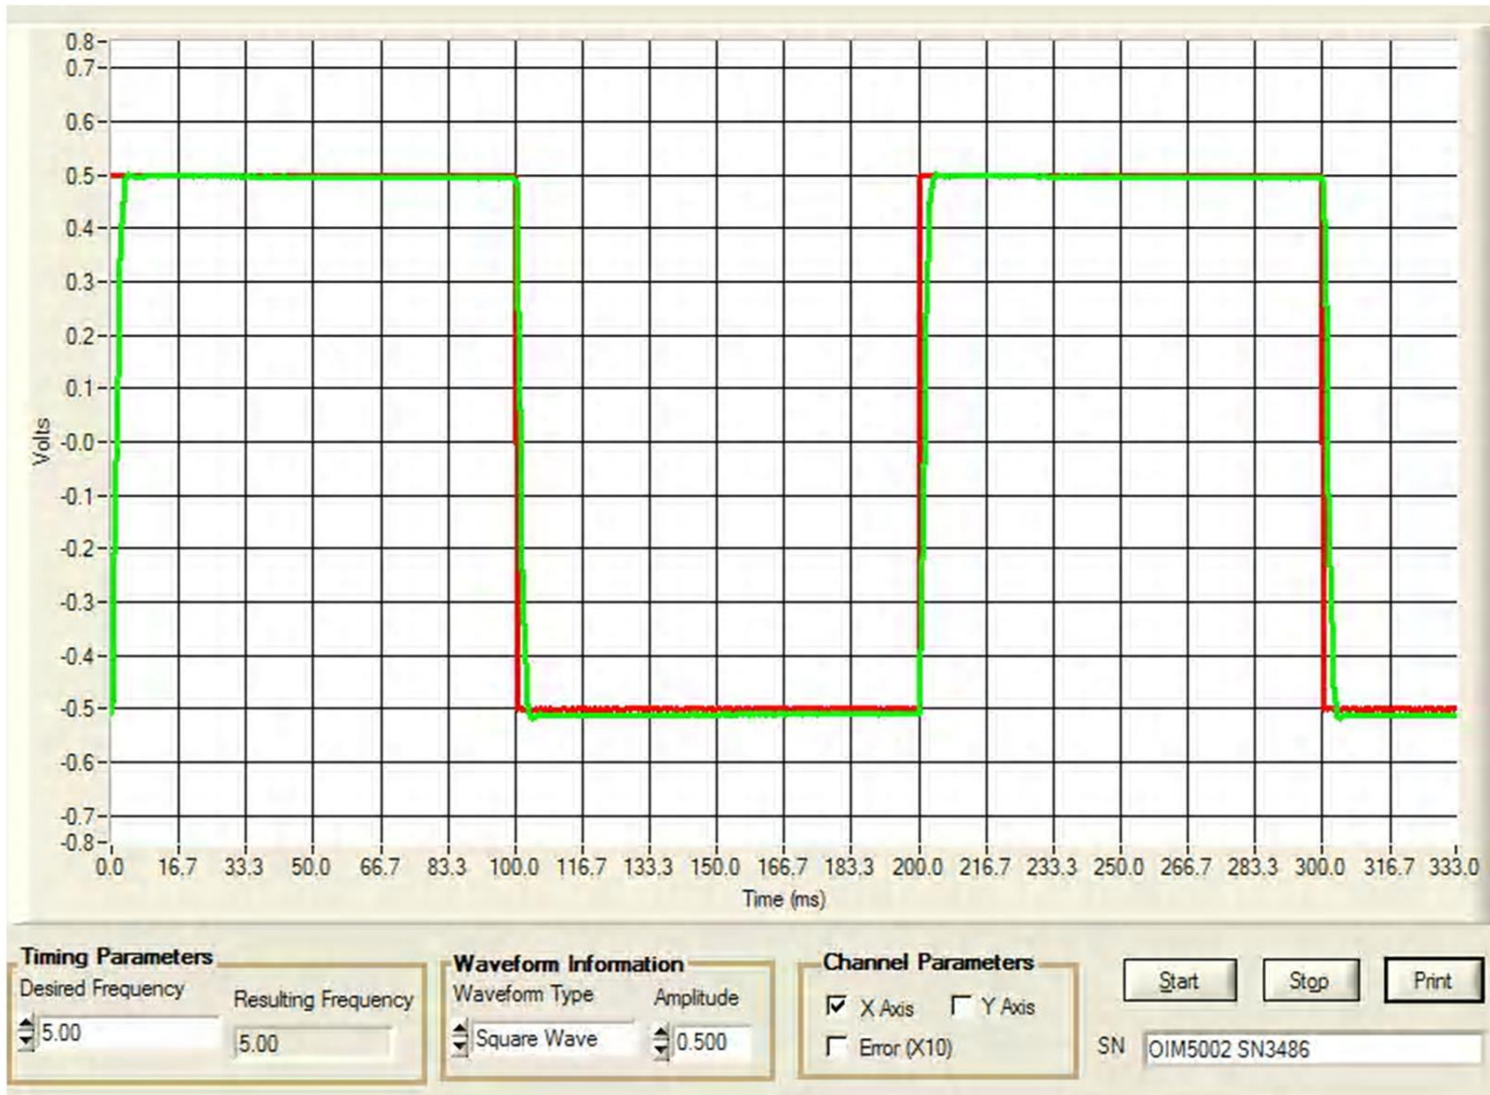

OIM5002 SN3486 Med Step X

Thursday, February 02, 2017


4:21 PM

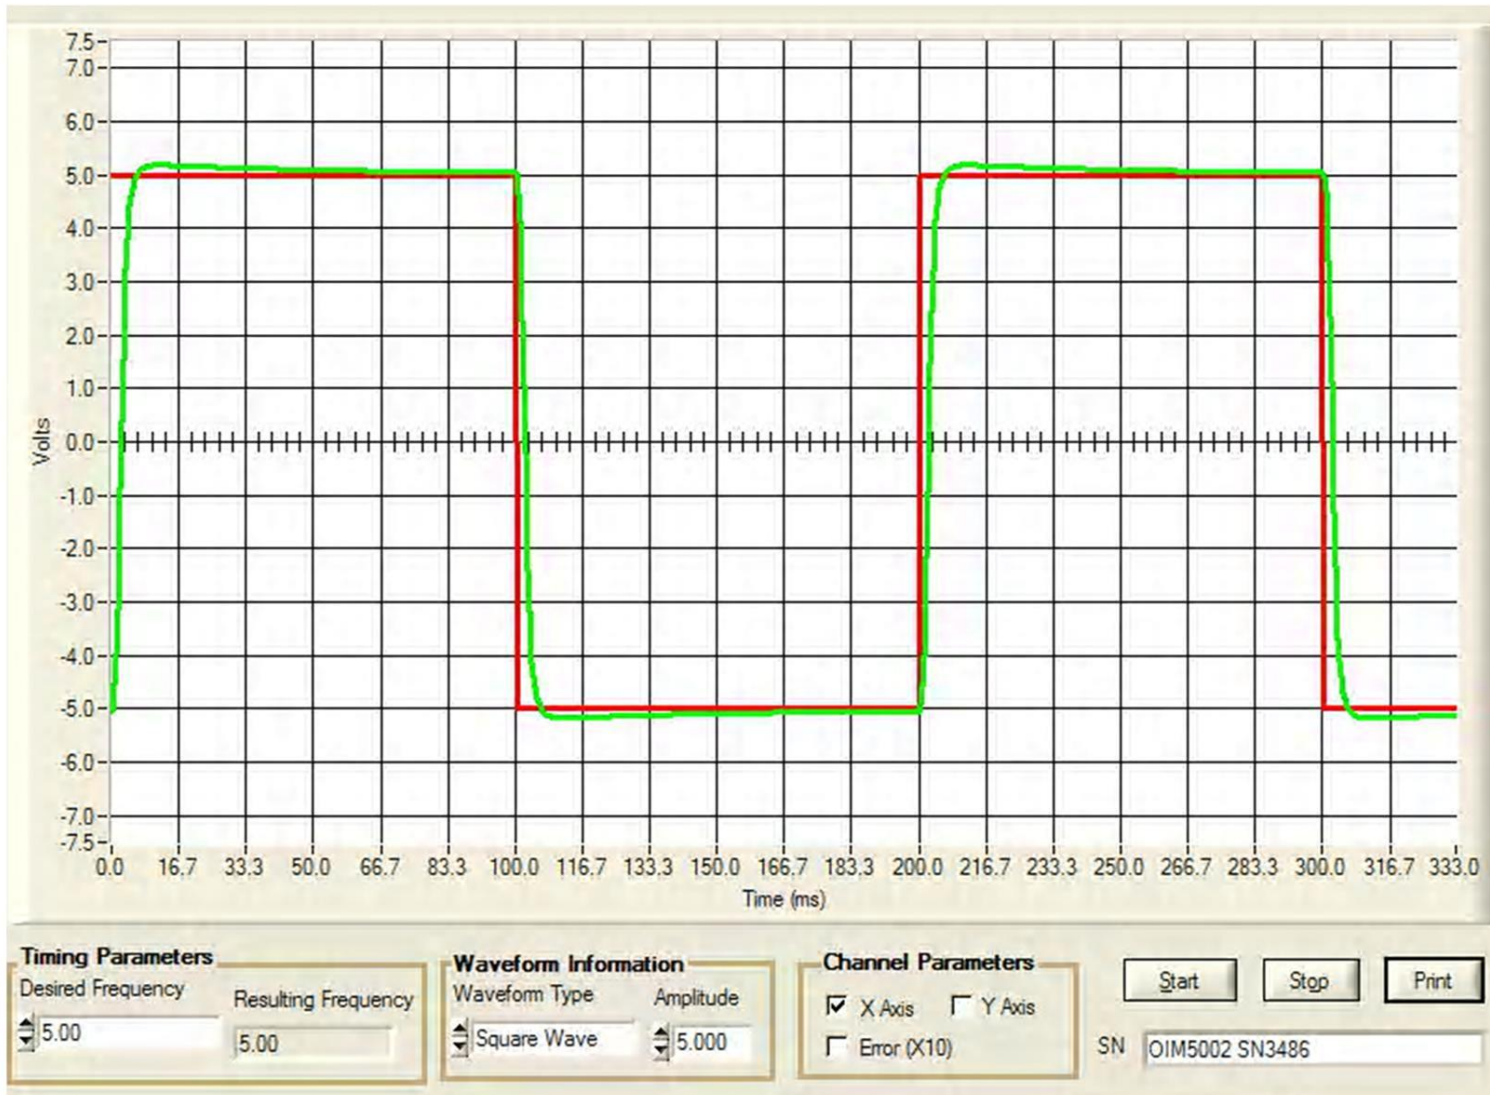

OIM5002 SN3486 Large Step X

Thursday, February 02, 2017


4:22 PM

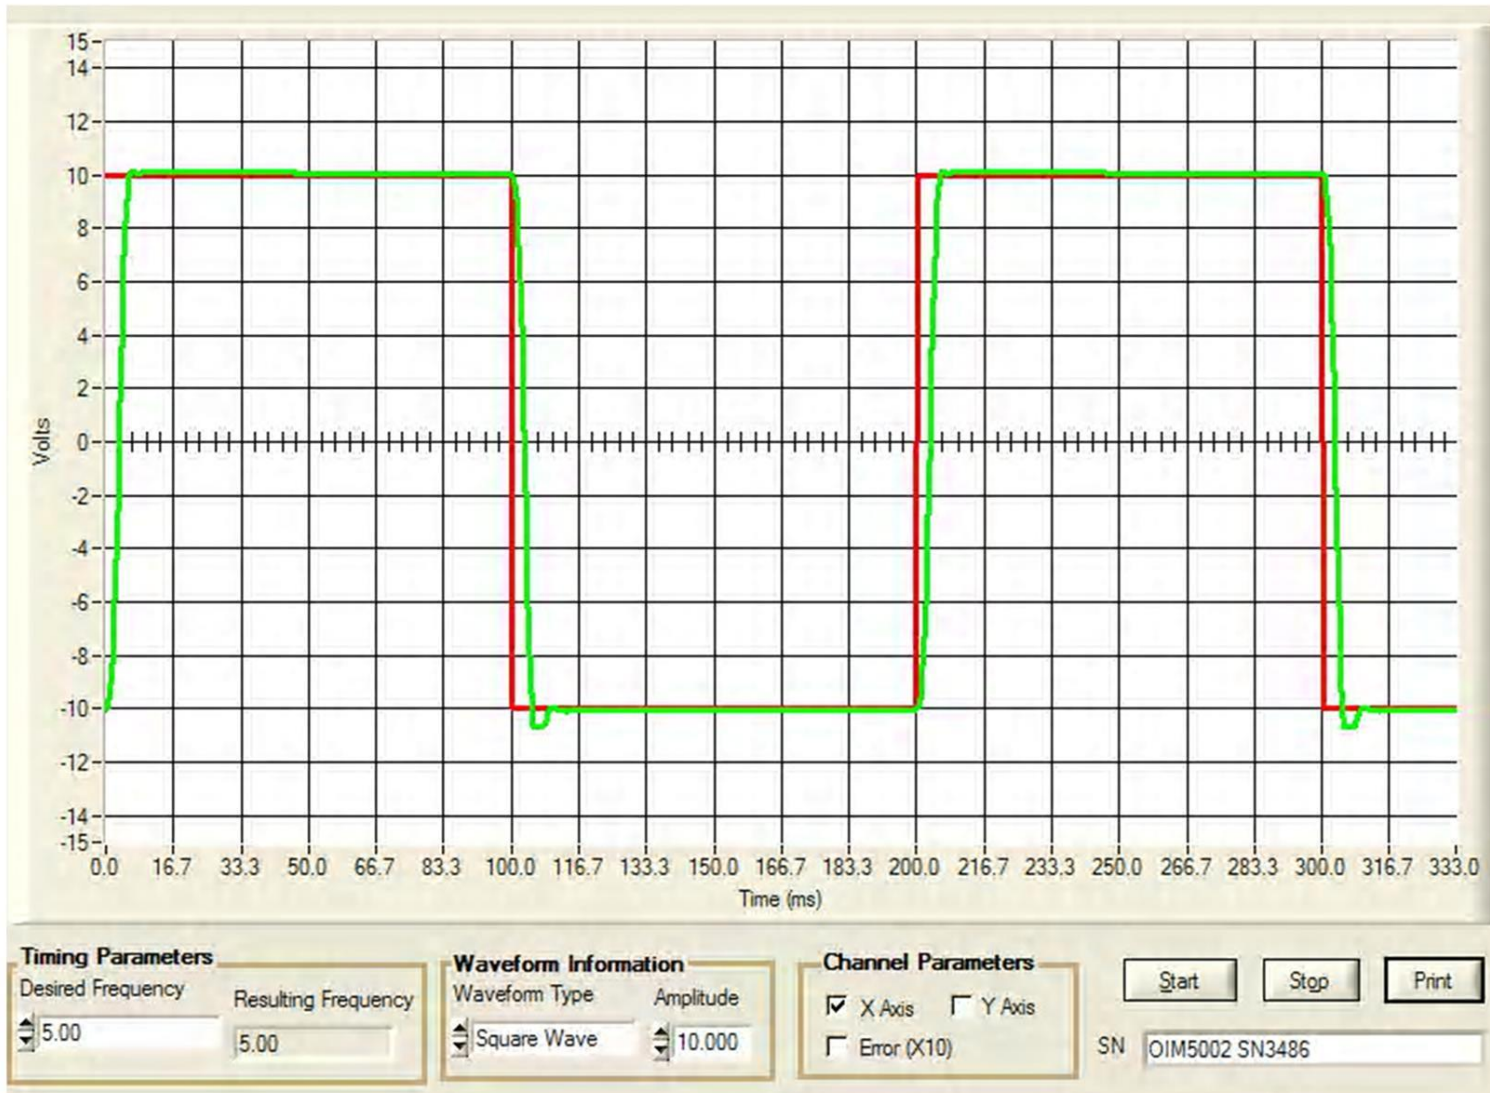

OIM5002 SN3486 Small Step Y

Thursday, February 02, 2017


4:22 PM

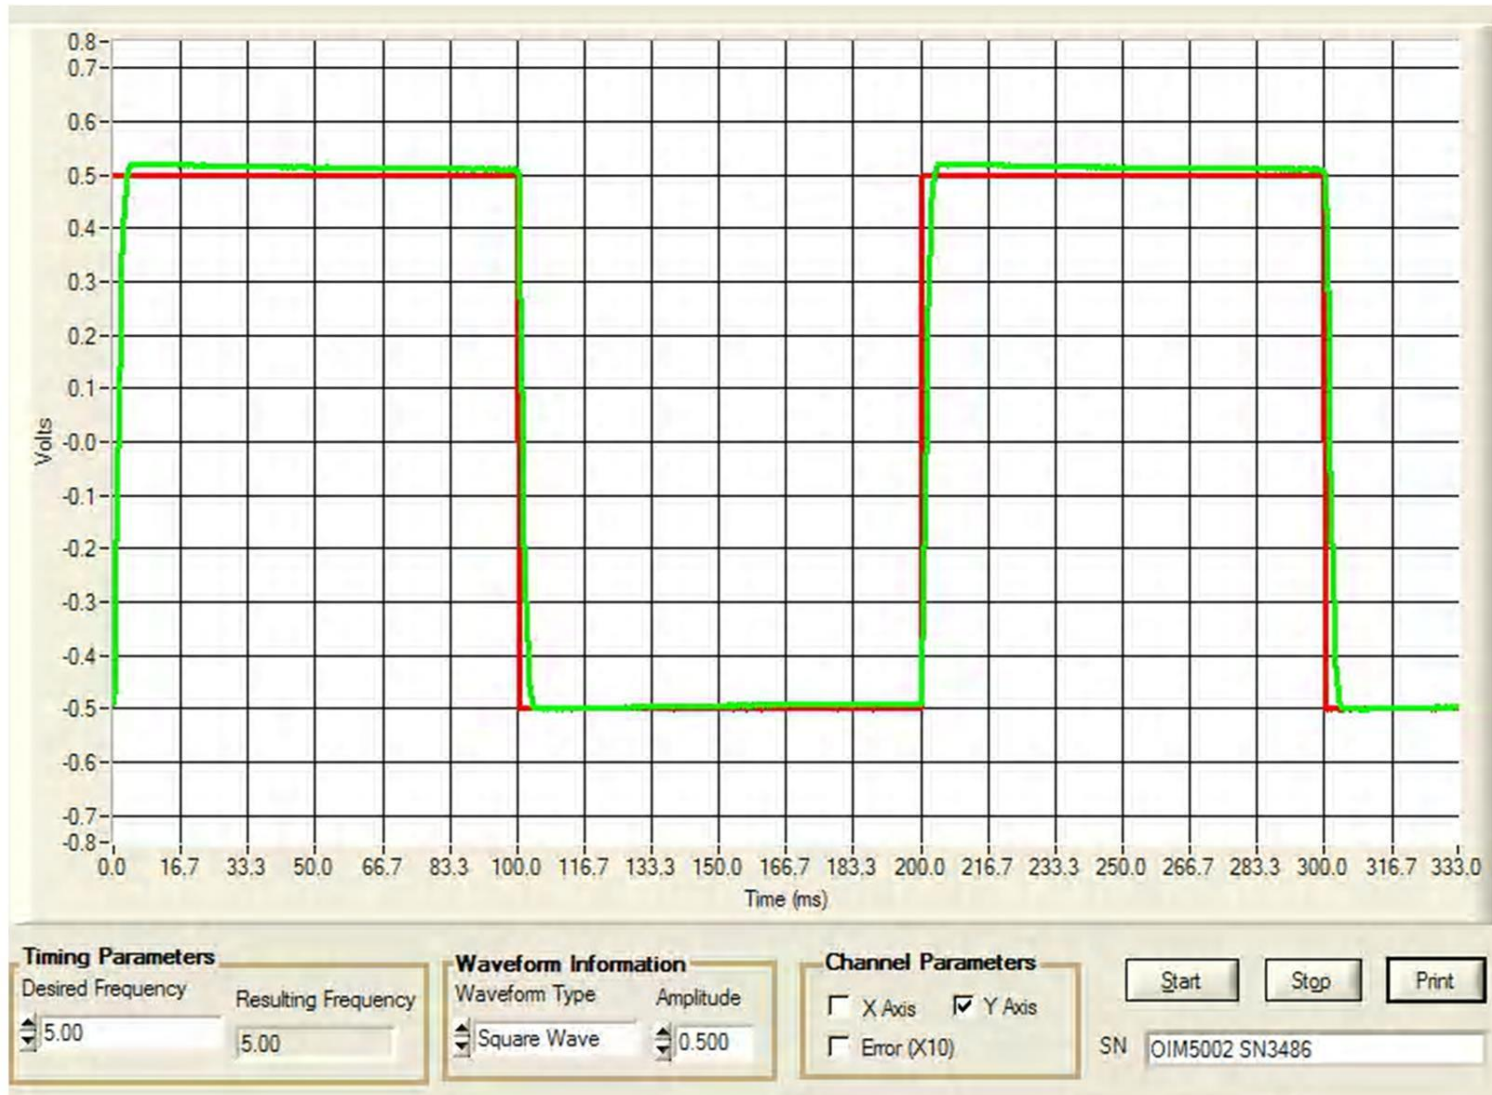

OIM5002 SN3486 Med Step Y

Thursday, February 02, 2017


4:22 PM

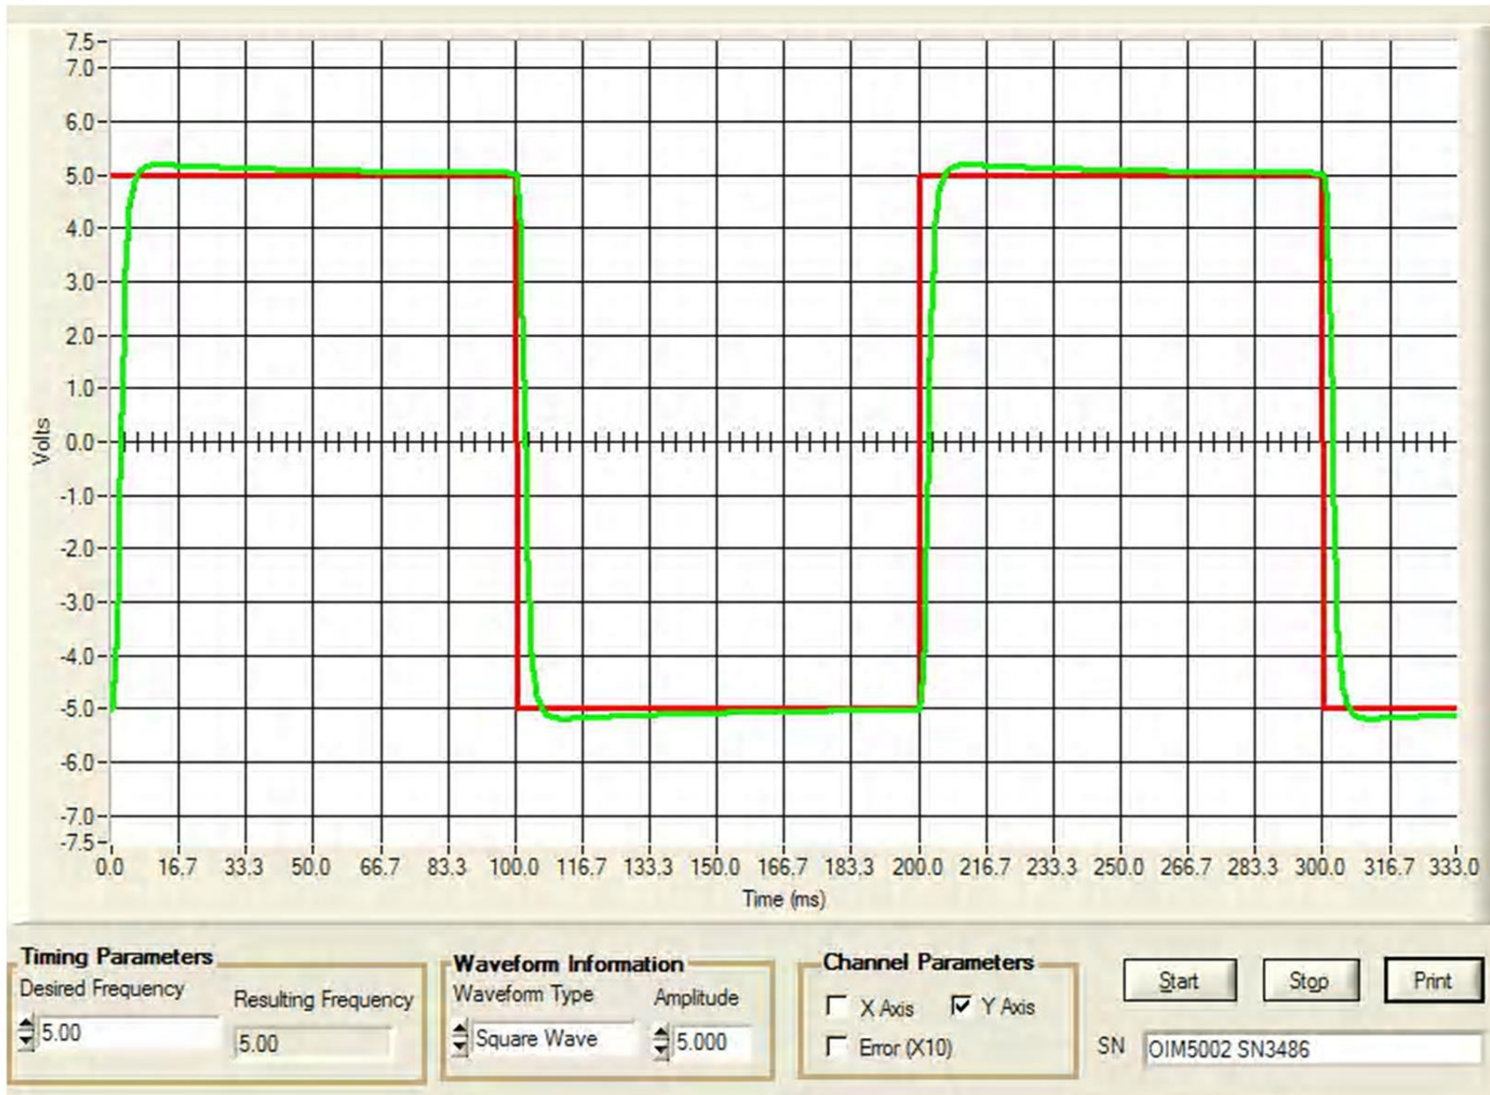

OIM5002 SN3486 Large Step Y

Thursday, February 02, 2017


4:22 PM

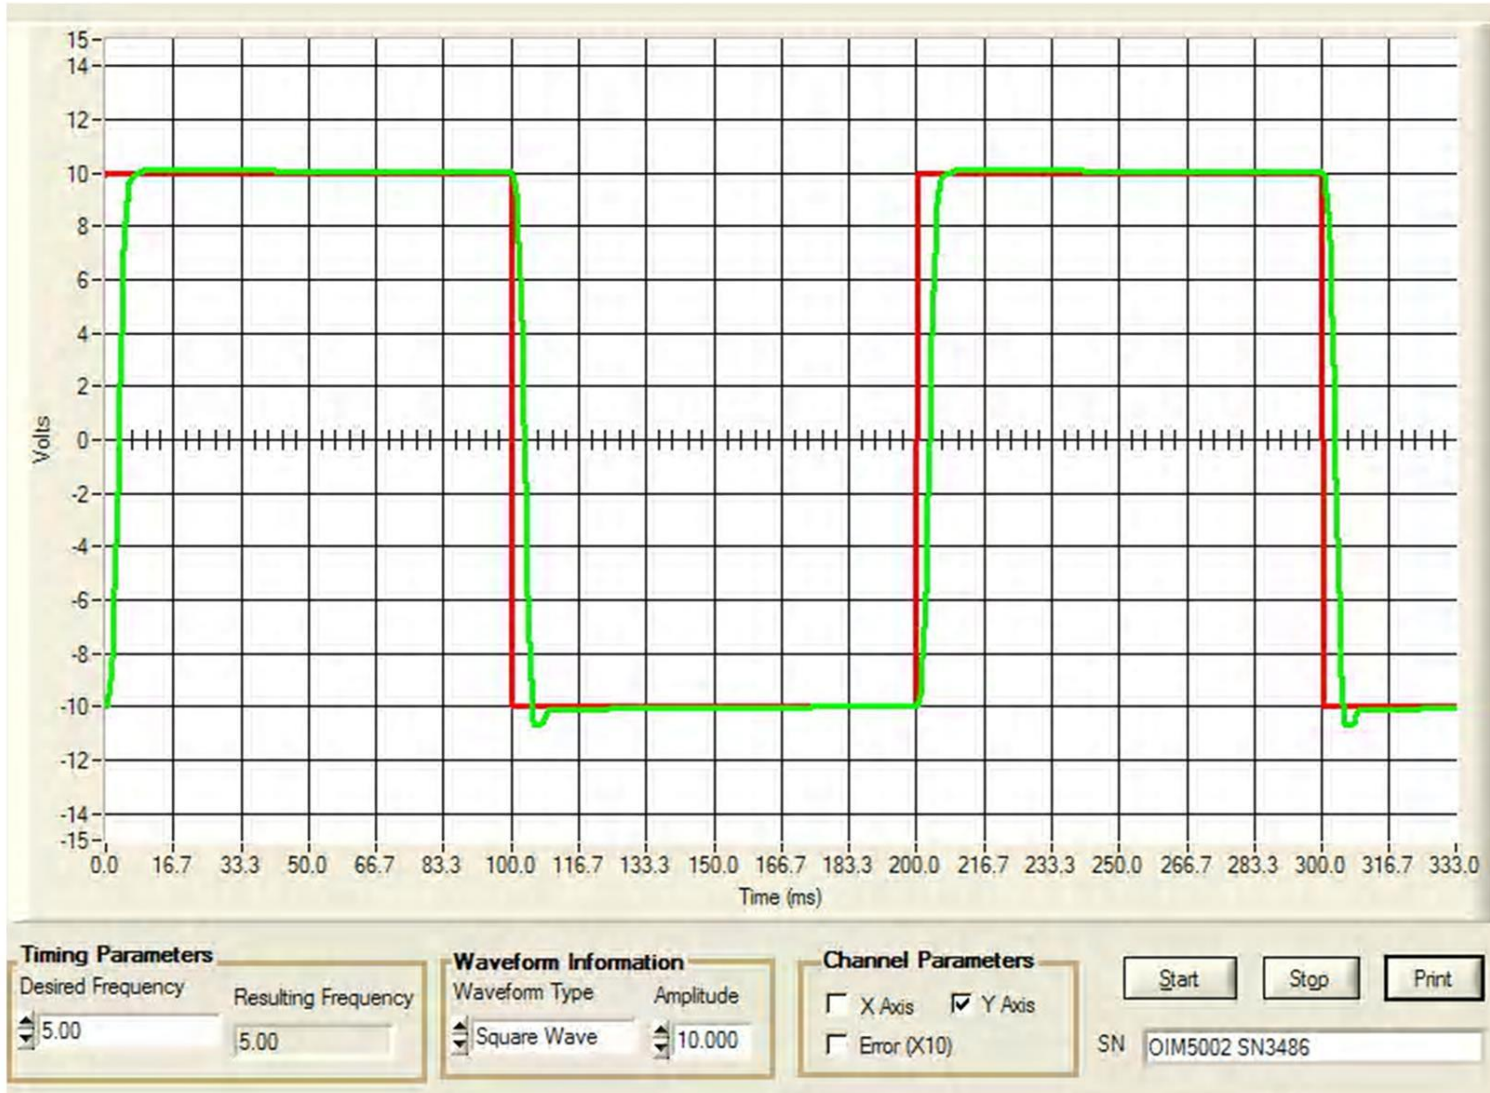

OIM5002 SN3487 Bode X

Thursday, February 02, 2017

5:12 PM

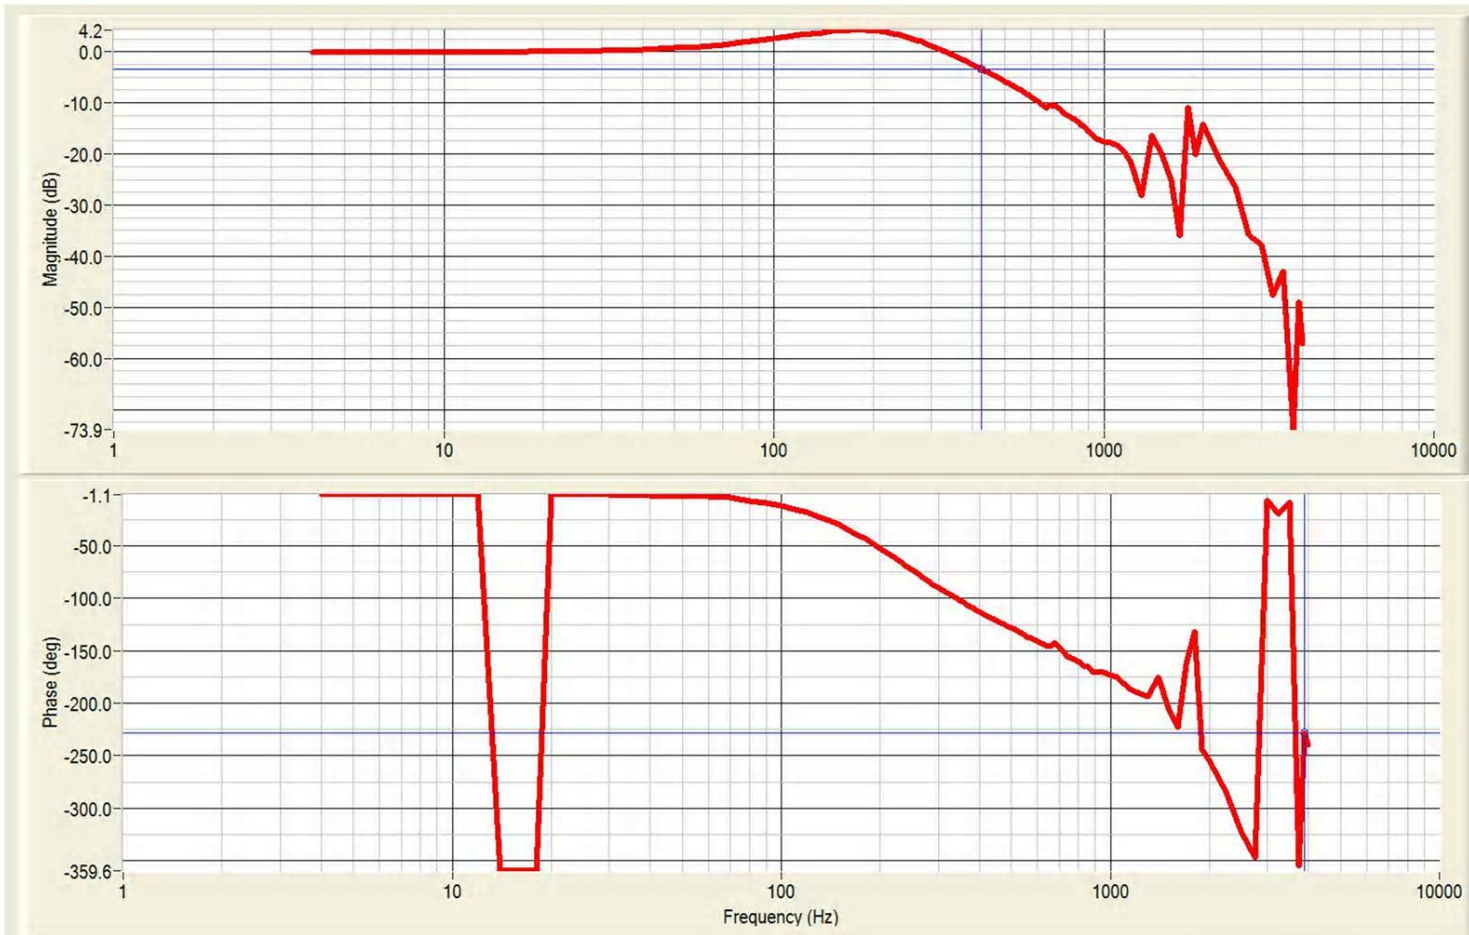

Closed Loop Error Rejection Open Loop

SN

Frequency	Magnitude	Phase
<input type="text" value="4000.000"/>	<input type="text" value="-57.122"/>	<input type="text" value="-239.761"/>

X Axis Y Axis

START

PRINT

Cursor Position


Frequency (Hz)	Magnitude (dB)
<input type="text" value="425.000"/>	<input type="text" value="-3.399"/>

Frequency (Hz)	Phase (deg)
<input type="text" value="0.000"/>	<input type="text" value="0.000"/>

OIM5002 SN3487 Bode Y

Thursday, February 02, 2017

5:14 PM

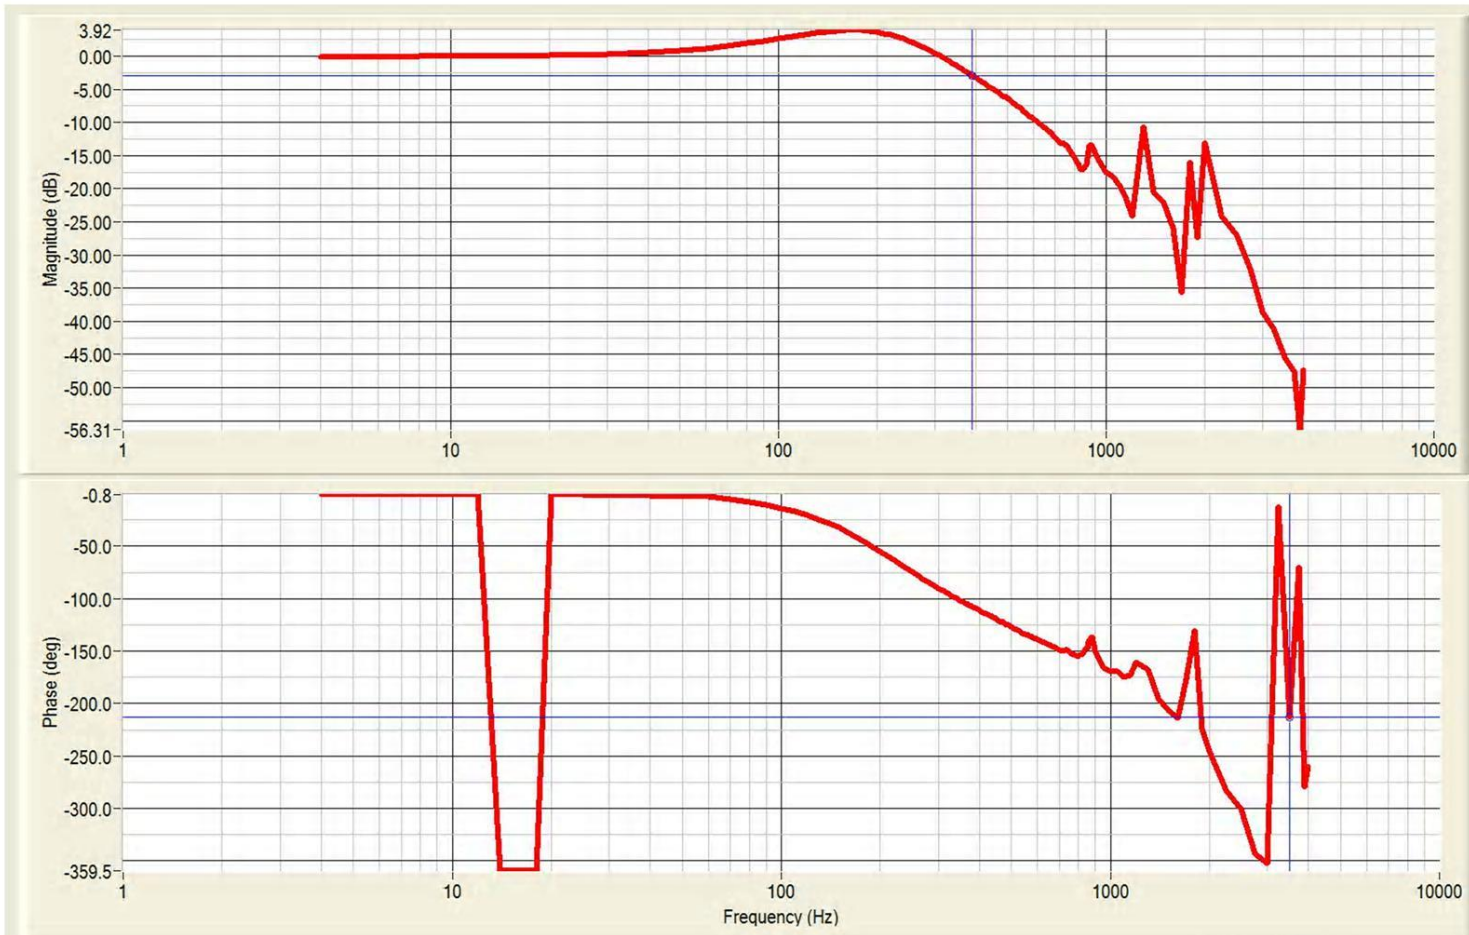

Cursor Position

Frequency (Hz)	Magnitude (dB)
390.000	-2.933
Frequency (Hz)	Phase (deg)
0.000	0.000

Closed Loop Error Rejection Open Loop

SN

Frequency	Magnitude	Phase
4000.000	-47.382	-260.377

X Axis Y Axis


START

PRINT

OIM5002 SN3487 Small Step X

Thursday, February 02, 2017


5:15 PM

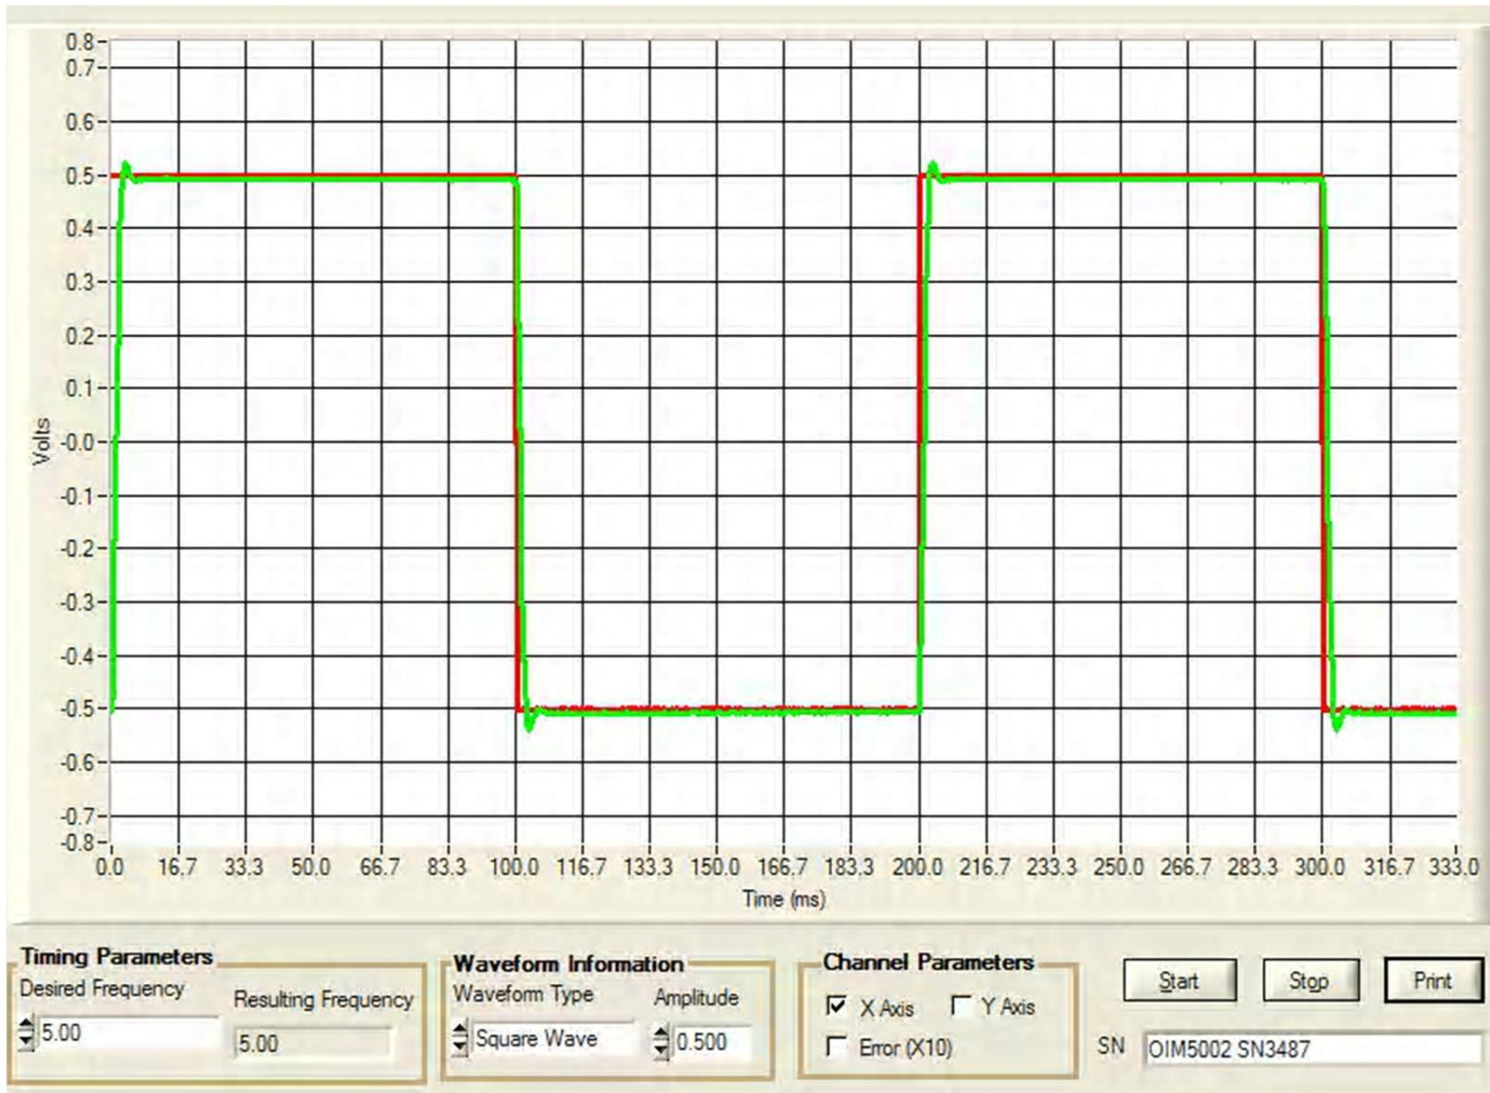

OIM5002 SN3487 Med Step X

Thursday, February 02, 2017


5:15 PM

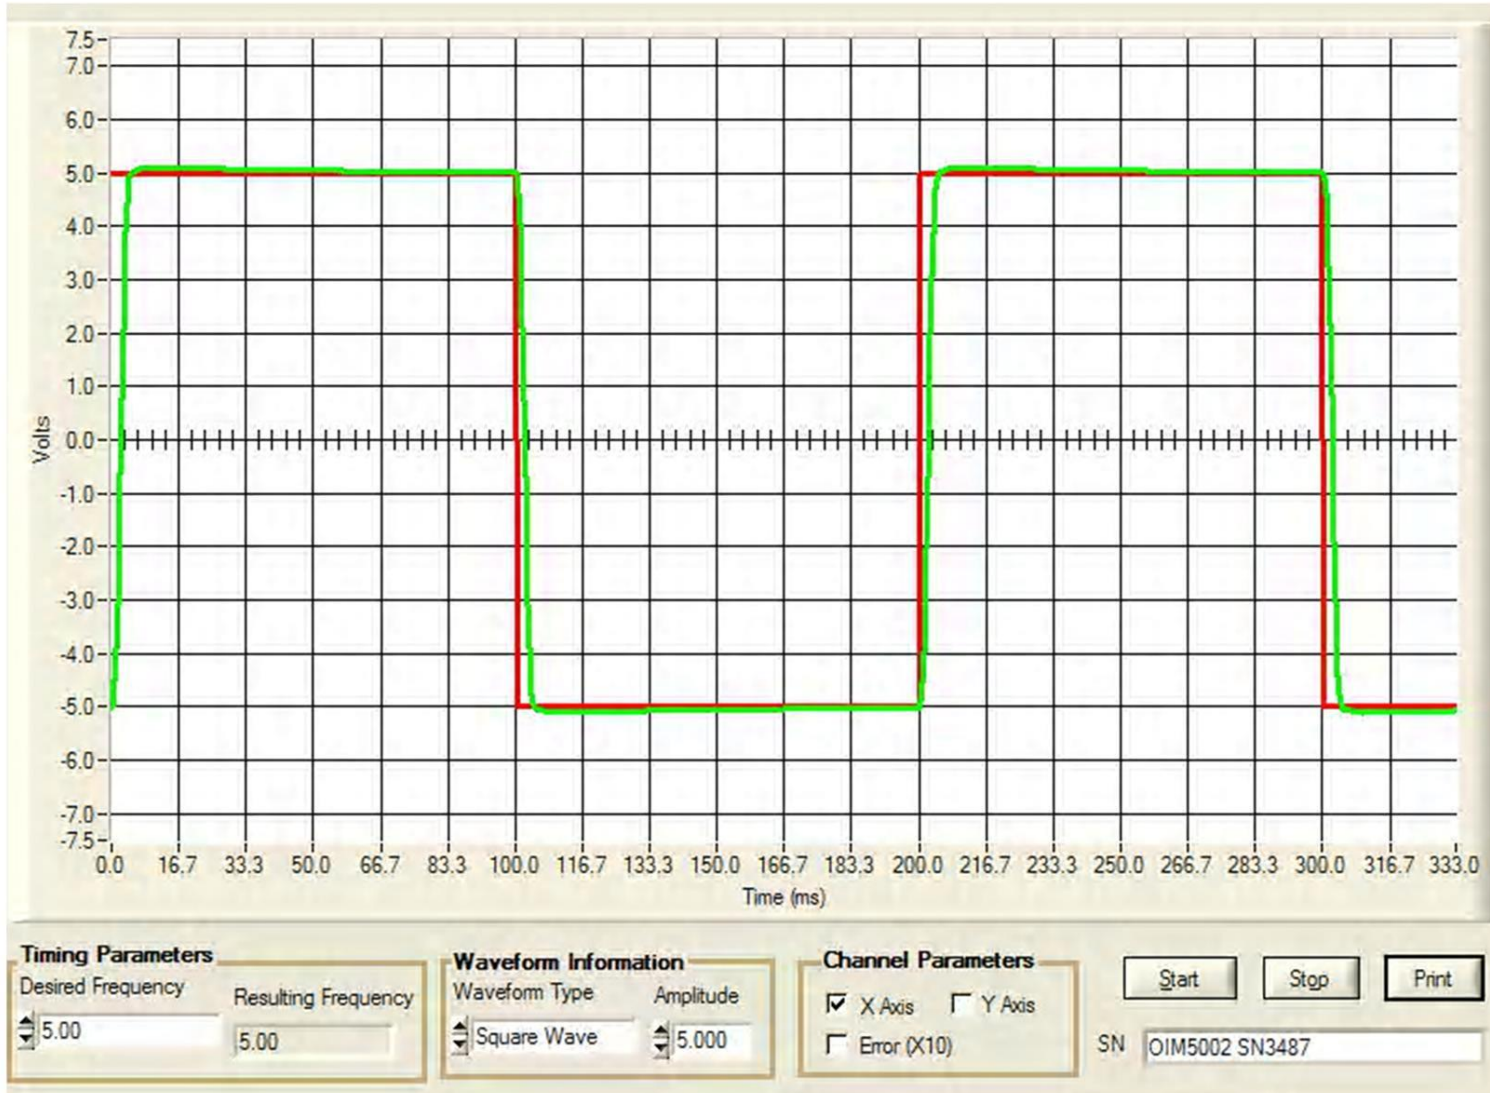

OIM5002 SN3487 Large Step X

Thursday, February 02, 2017


5:15 PM

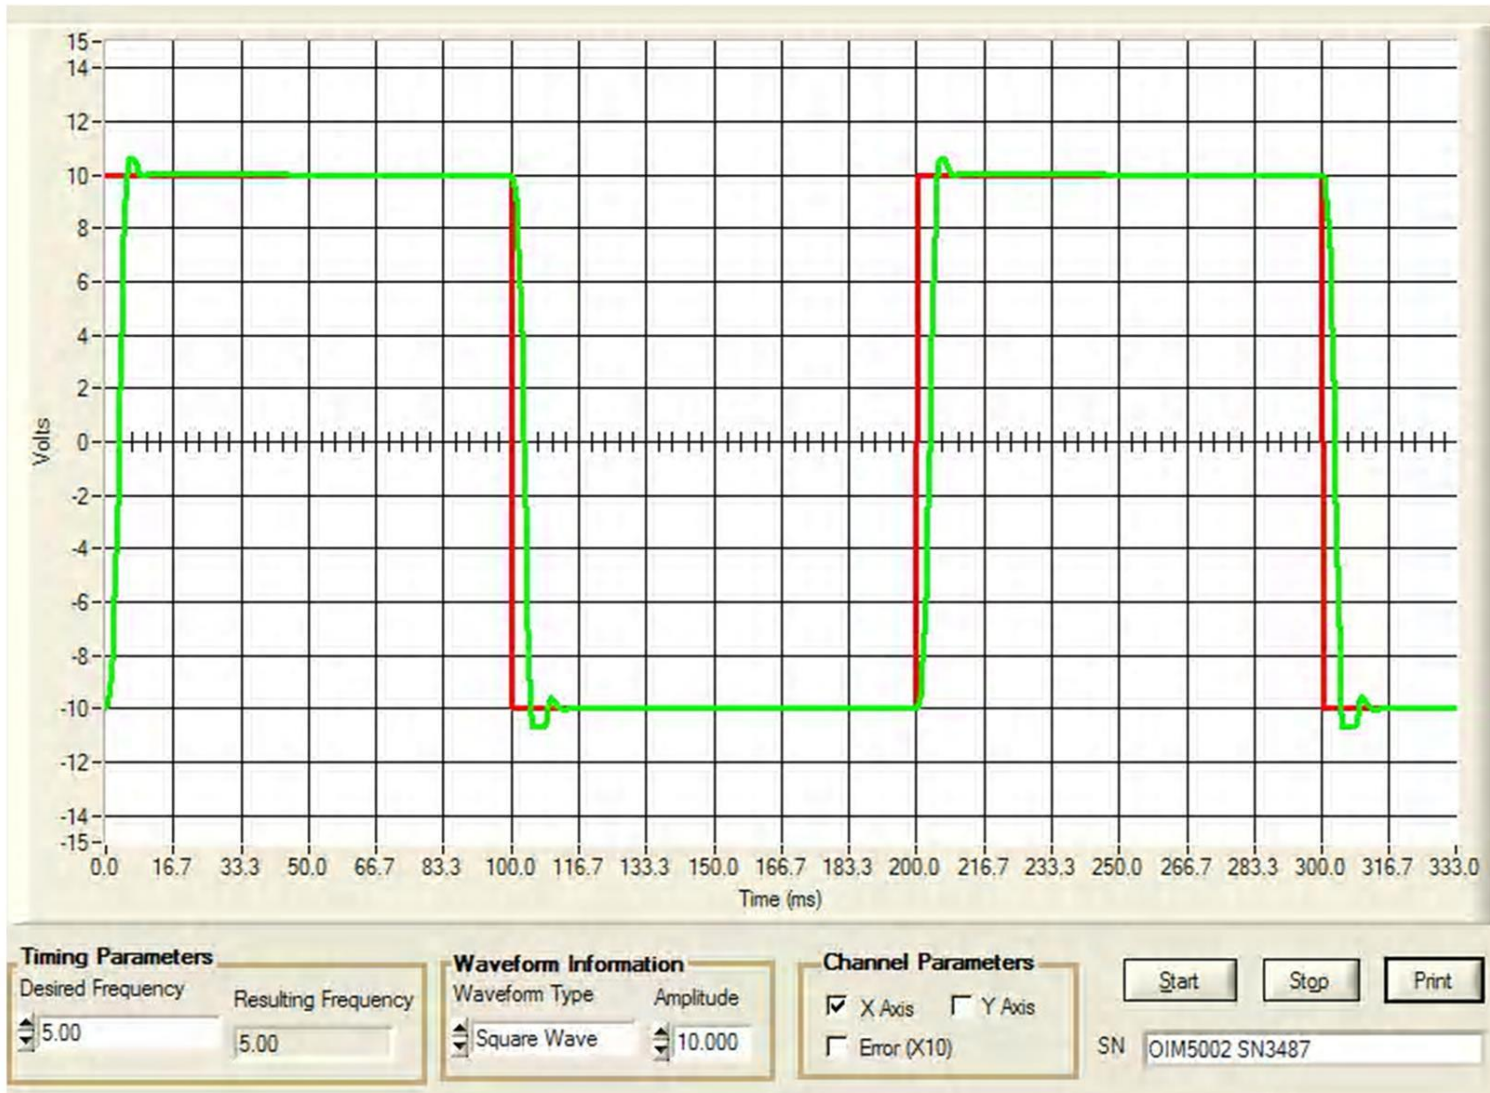

OIM5002 SN3487 Small Step Y

Thursday, February 02, 2017


5:16 PM

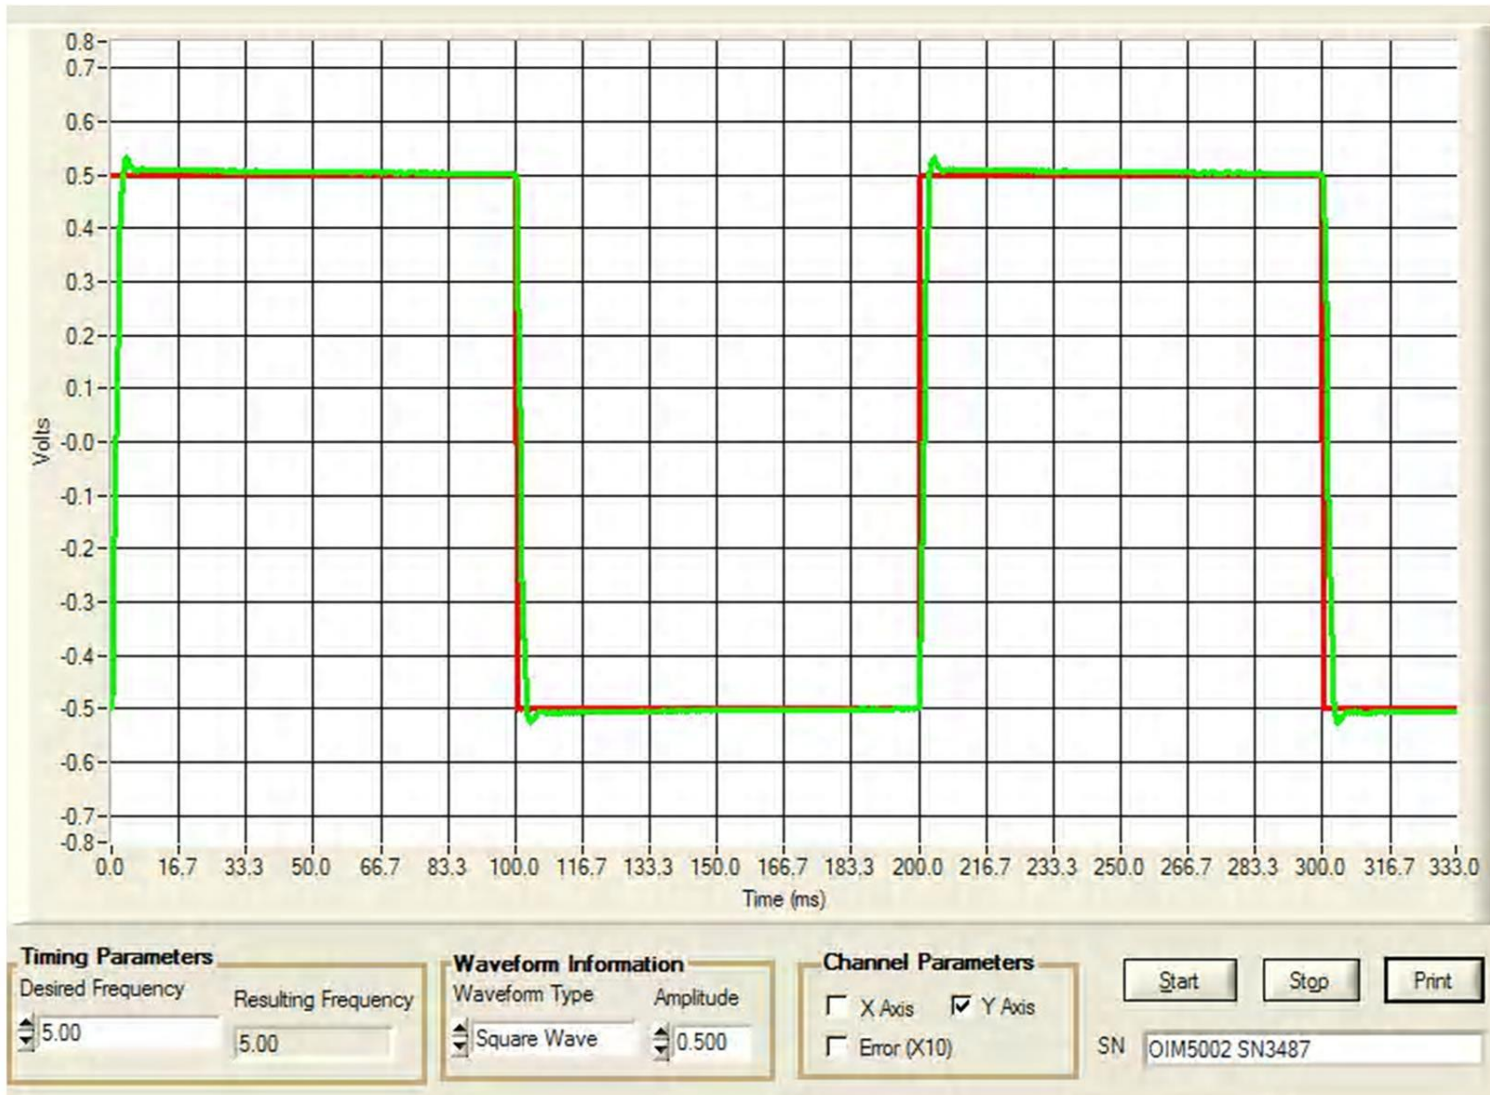

OIM5002 SN3487 Med Step Y

Thursday, February 02, 2017

5:16 PM

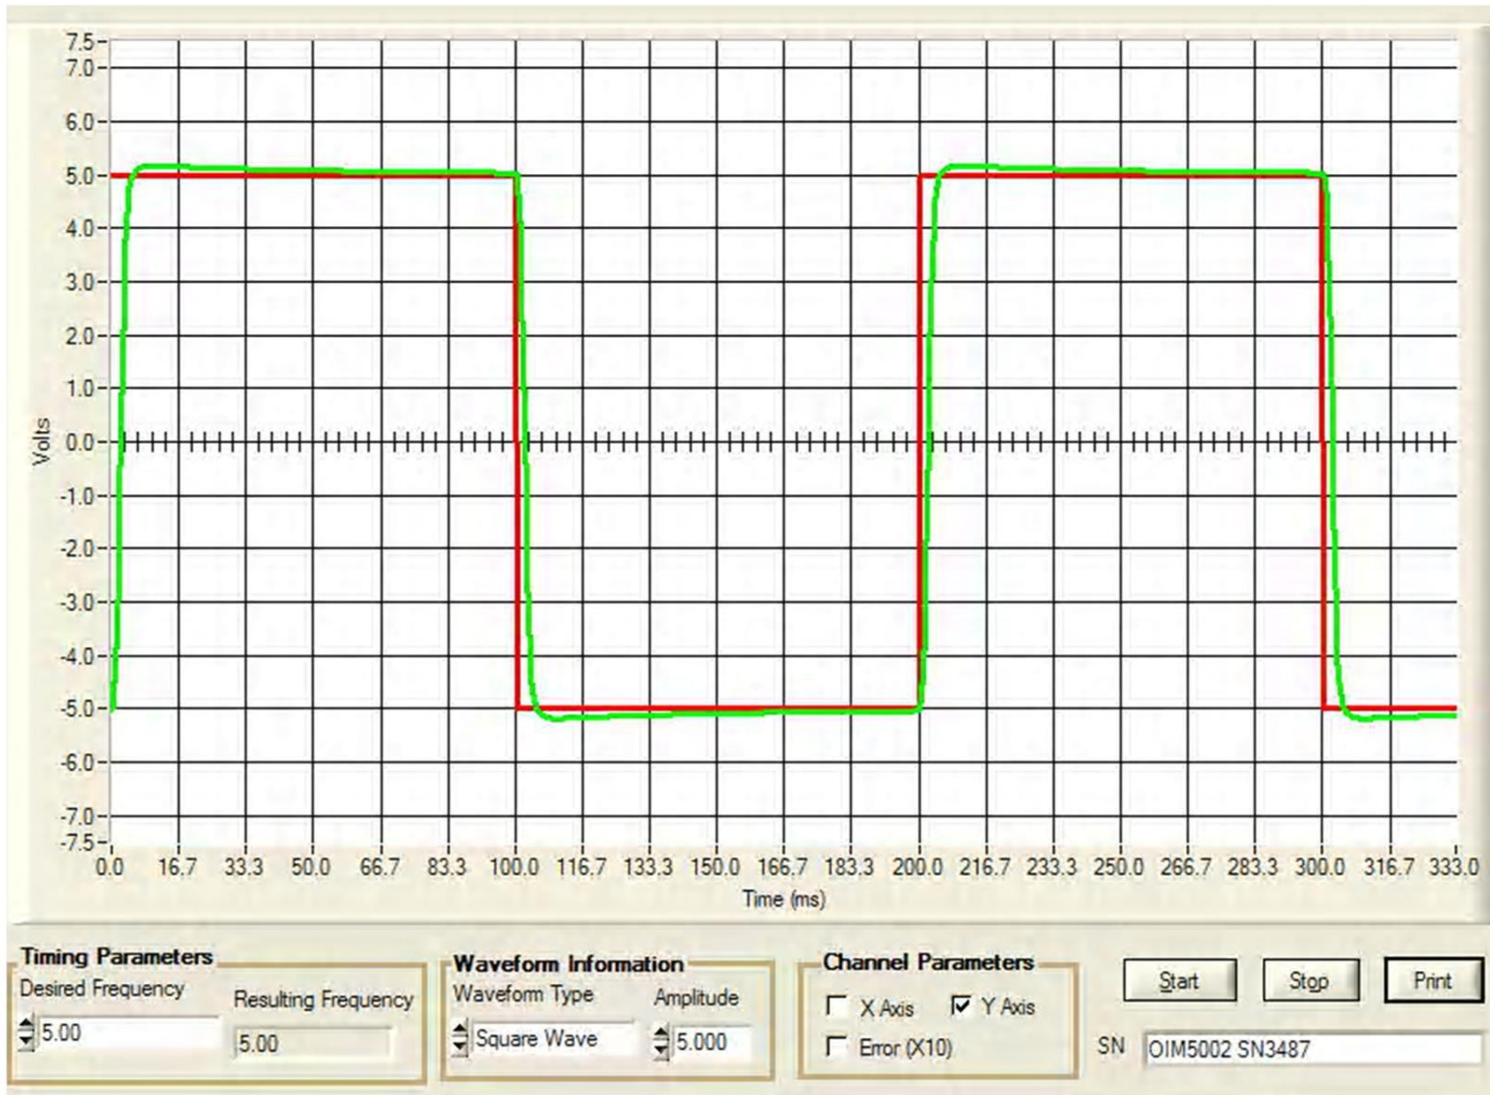

OIM5002 SN3487 Large Step Y

Thursday, February 02, 2017

5:16 PM

